

CORRECTION

Open Access




Correction: Evaluating the consistency in different methods for measuring left atrium diameters

Jun-Yan Yue^{1,2,3}, Kai Ji¹, Hai-Peng Liu¹, Qing-Wu Wu¹, Chang-Hua Liang¹ and Jian-Bo Gao^{2*}

Correction: Yue et al. *BMC Medical Imaging* (2024) 24:57.
<https://doi.org/10.1186/s12880-024-01231-6>

In the original article [1], Figure 3 was incorrectly duplicated from Figure 6 during the typesetting process.

The wrong Figure 3 is shown below:

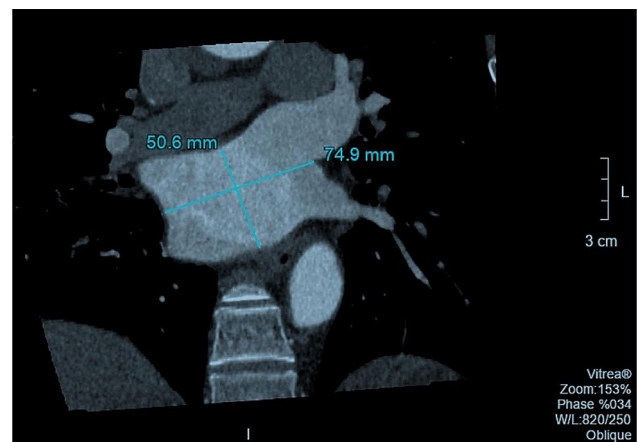

The online version of the original article can be found at <https://doi.org/10.1186/s12880-024-01231-6>.

*Correspondence:

Jian-Bo Gao
gaojianbo3762@163.com

¹Department of Radiology, The First Affiliated Hospital of Xinxiang Medical University, Weihui Henan Province, 453200 Xinxiang, China


²Department of Radiology, The First Affiliated Hospital of Zhengzhou University, No. 1 Jianshe East Road, Erqi District, 450000 Zhengzhou, Henan Province, China

³Heart Center, The First Affiliated Hospital of Xinxiang Medical University, 453200 Henan Province, Weihui, China



© The Author(s) 2024. **Open Access** This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>. The Creative Commons Public Domain Dedication waiver (<http://creativecommons.org/publicdomain/zero/1.0/>) applies to the data made available in this article, unless otherwise stated in a credit line to the data.

The correct Figure 3 is shown below:

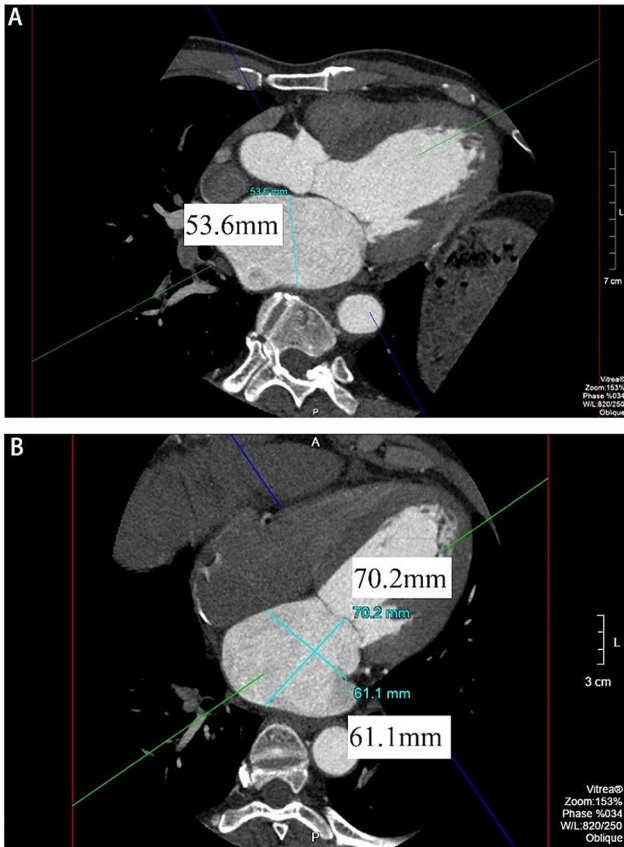

The original article [1] has been corrected.

Published online: 08 April 2024

References

1. Yue JY, Ji K, Liu HP, et al. Evaluating the consistency in different methods for measuring left atrium diameters. BMC Med Imaging. 2024;24:57. <https://doi.org/10.1186/s12880-024-01231-6>.

Publisher's Note

Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.